


Parteneriat pentru un viitor mai bun
www.interreg-rohu.eu

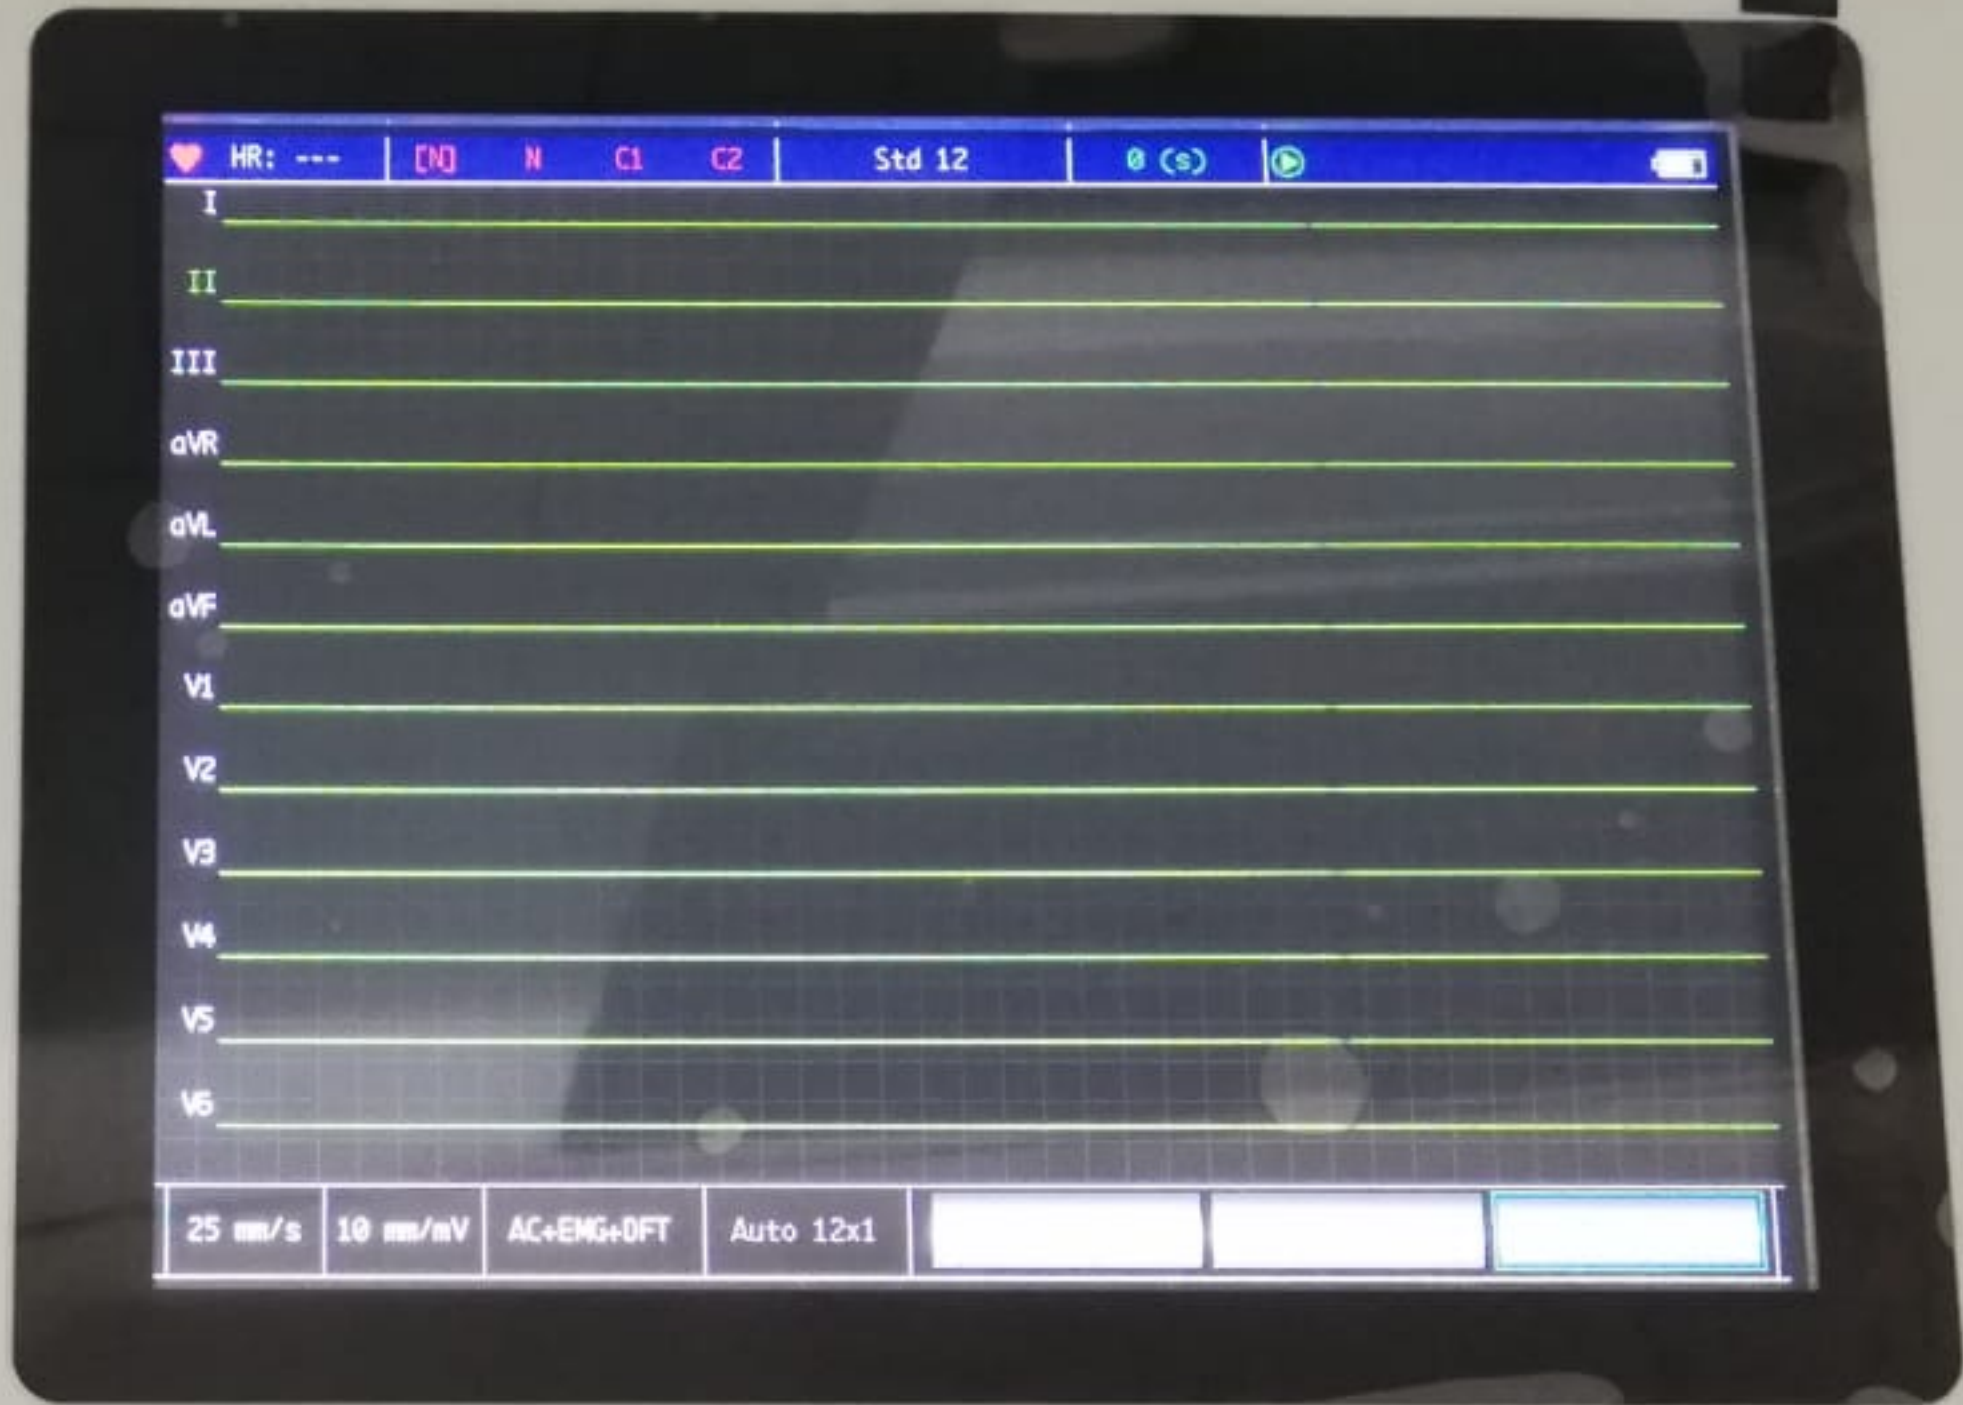

DANGER Possible explosion hazard if used in the presence of flammable anesthetics

↓/⏻ ⏻ ON/OFF


1	2	3	4	5	←	↑	
ABC	DEF	GHI	JKL	Backspace	←	OK	→
6	7	8	9	0	↻	↓	
MNO	PQRS	TUV	WXYZ	└	1-a-A		

mm/s SPEED FILTER PRINT START/STOP

SEN MODE

Control panel of a medical device with the following buttons and labels:

- STOP (orange circle with a square)
- START (blue circle with a square)
- MODE (envelope icon)
- PRINT (printer icon)
- MM/s (speed unit)
- MINO (6)
- MINO (7)
- MINO (8)
- MINO (9)
- MINO (0)
- 1 (1)
- 2 (2)
- 3 (3)
- 4 (4)
- 5 (5)
- OK (center)
- Navigation arrows (up, down, left, right)
- ON/OFF (bottom left)
- Backspace (left of 1-5)
- 1-5 (top of 1-5)
- WXYZ (top of 6-9)
- ABC (top of 1-5)
- DEF (top of 3-5)
- GHI (top of 4-5)
- JKL (top of 5)

 DANGER Possible explosion hazard if used in the presence of flammable anesthetics





 **Interreg**
România-Ungaria
Parteneriat pentru dezvoltare regională

Parteneriat pentru un viitor mai bun
www.interreg-romania.ro

Parteneriat pentru un viitor mai bun
www.interreg-rohu.eu


Interreg
România - Ungaria
Fondul European de Dezvoltare Regională

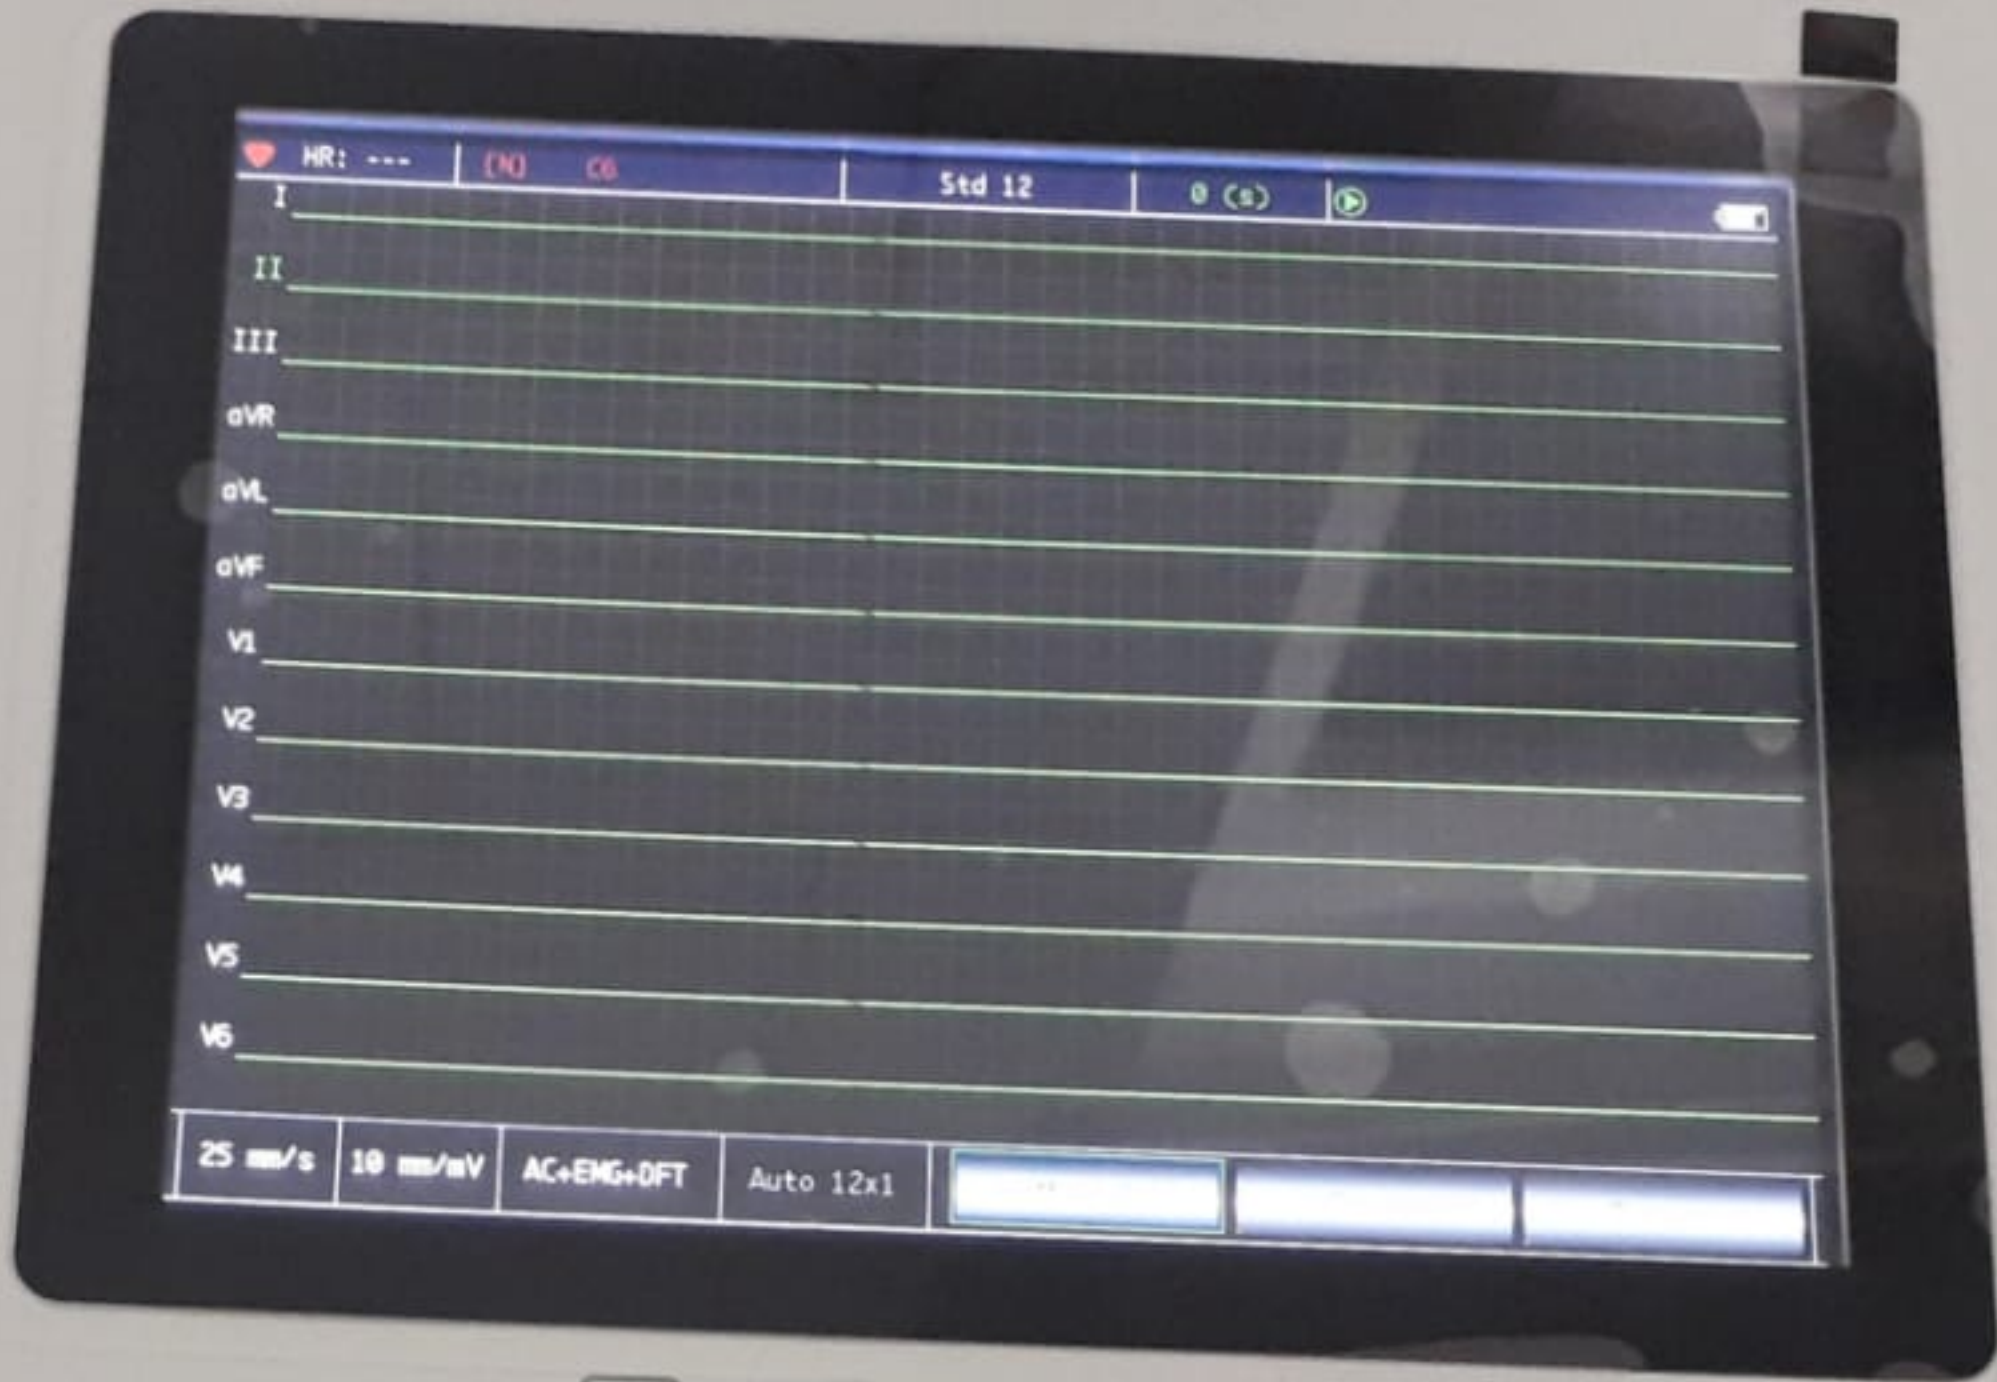

 DANGER Possible explosion hazard if used in the presence of flammable anesthetics

V/A   ON/OFF

1	2 ABC	3 DEF	4 GHI	5 JKL	 Backspace	
6 MNO	7 PQRS	8 TUV	9 WXYZ	0]	 1-a-A	 OK 
 mm/s SPEED	 SEN	 FILTER	 MODE	 PRINT	 START	 STOP